How to manage a non-ENFit enteral device

Does the device have an equivalent ENFit product (ex: Mic-Key extension)?

Yes → Change device to ENFit version

If it is not possible to change the device, follow the rest of the algorithm

No

What needs to be administered?

Feed → **Use stepped connector**

Medication → **Use syringe adapter**
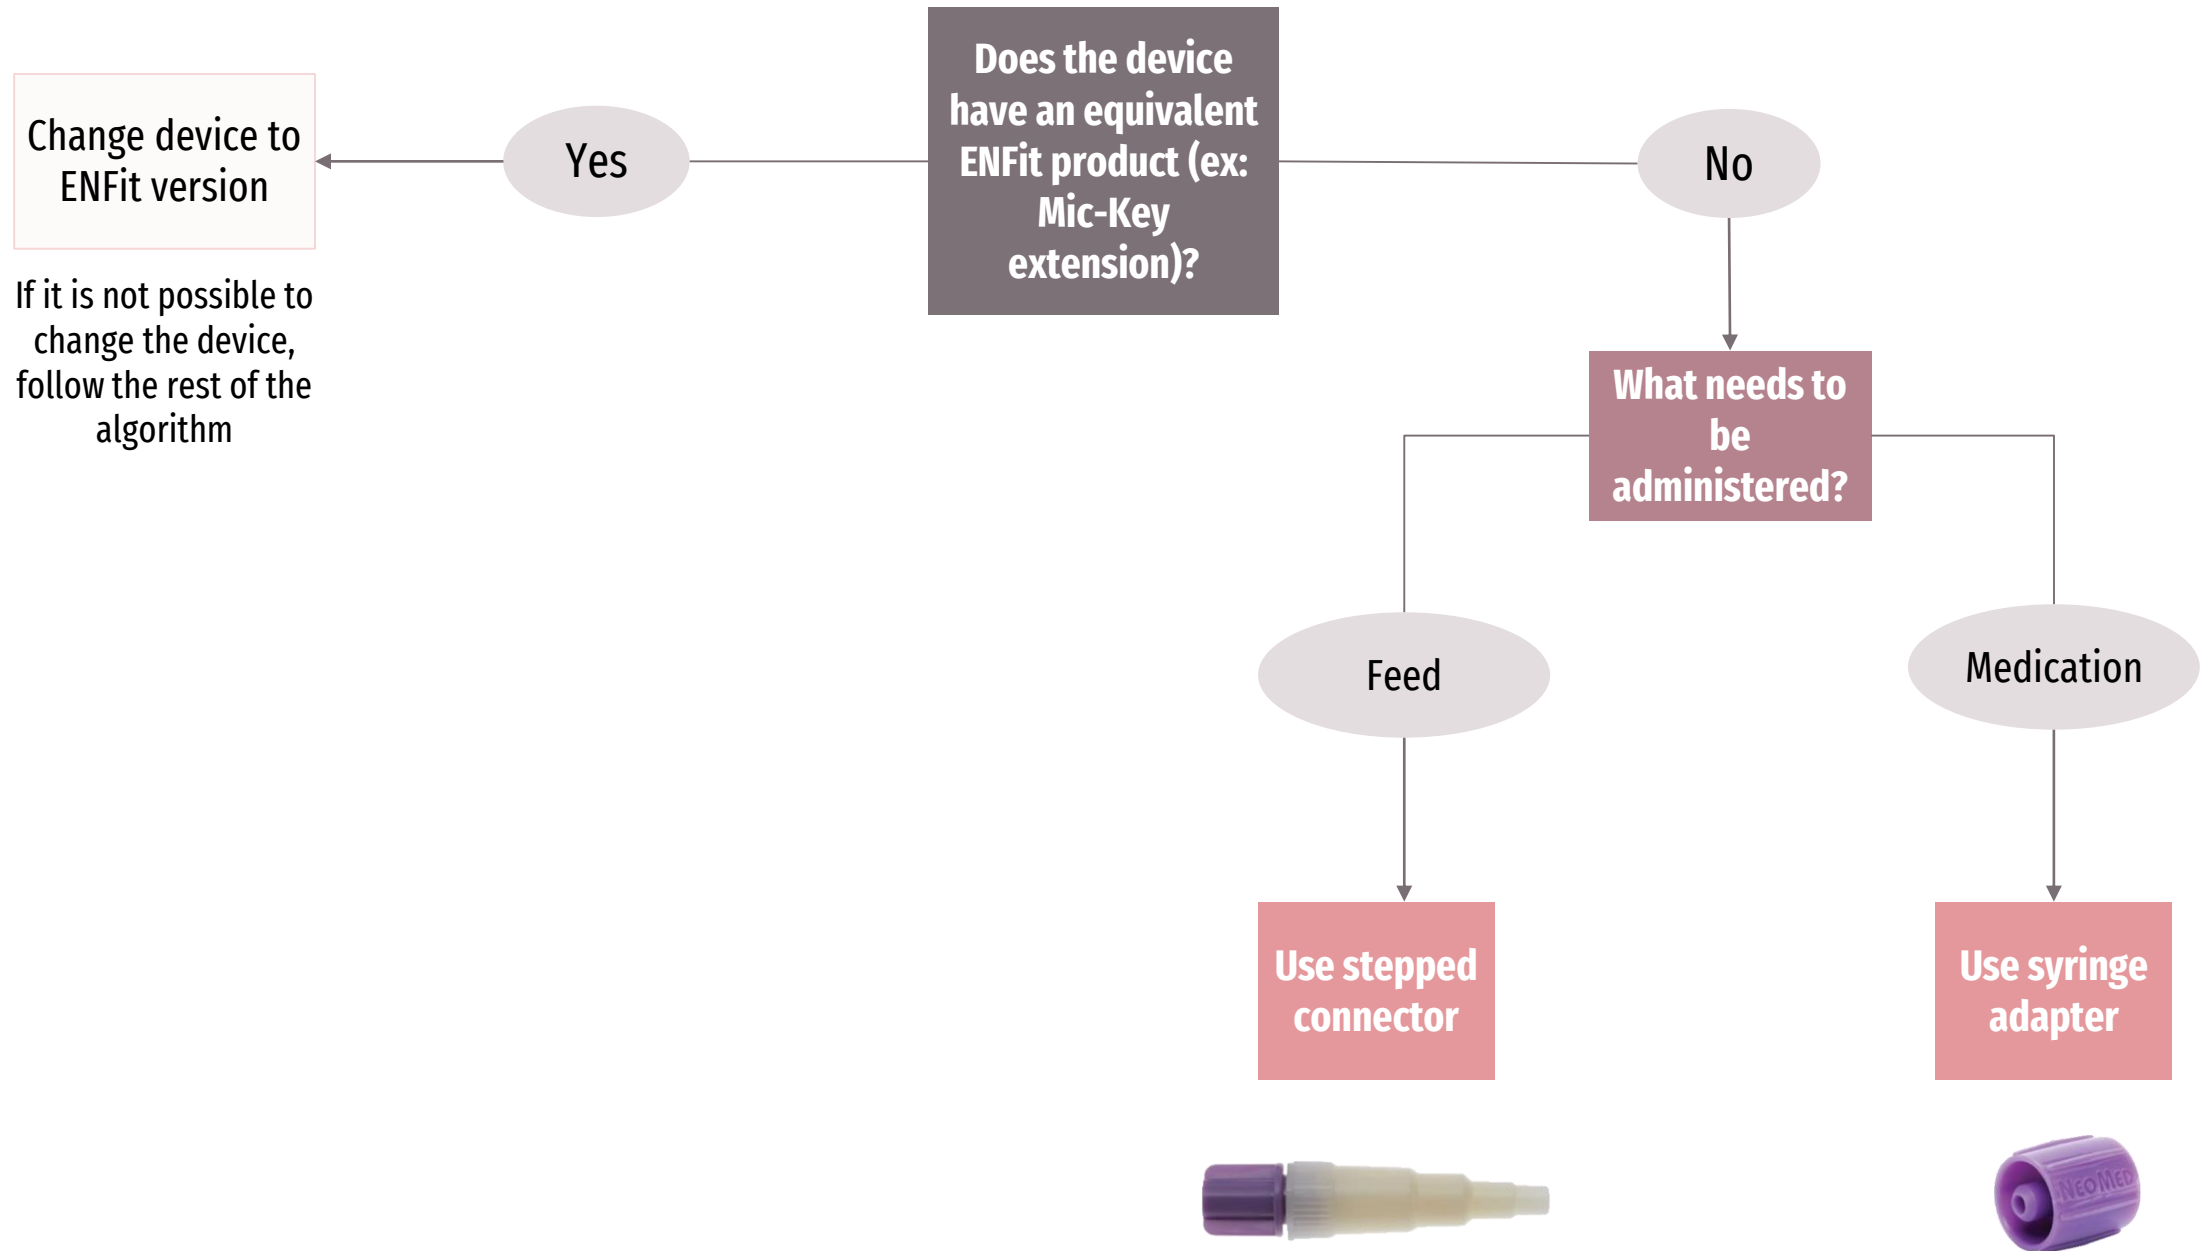
How to manage non-standard devices for enteral use

Use stepped connector ← Foley — **What is the product being used for?** — Replogle

What is it used for?

Decompression /suction → **Toomey syringe or luer-lock syringe (depends on size)**

Medication administration → **Use luer lock syringe**

Note: When using a non-standard device for enteral purposes, the team should consider switching to an ENFit device as soon as clinically feasible